


THE TOE SHOULD MOVE NOT THE IMPLANT

The HemiCAP® implant exhibits 375% LESS movement than a stemmed implant.*

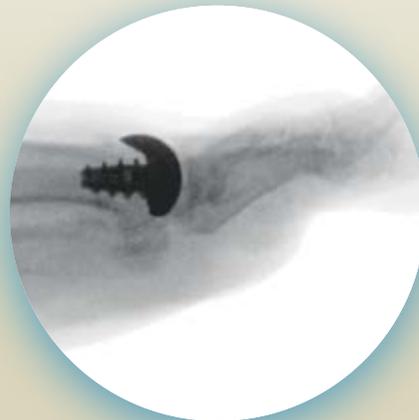

* In matched cadaveric specimens using simulated movement, the stemmed implant showed 4 times more displacement over the same 15,000 cycles as the HemiCAP® DF.